

OBSAH LAKTÓZY

Ranking of the laboratories

| Nb | N° | d | Sd | D |
|-----------|-----------|----------------|--------------|--------------|
| 1 | 26 | - 0.001 | 0.004 | 0.004 |
| 2 | 24 | - 0.008 | 0.006 | 0.010 |
| 3 | 4 | - 0.003 | 0.011 | 0.012 |
| 4 | 31 | + 0.000 | 0.012 | 0.012 |
| 5 | 15 | + 0.003 | 0.012 | 0.013 |
| 6 | 8 | - 0.006 | 0.014 | 0.015 |
| 7 | 5 | - 0.013 | 0.012 | 0.018 |
| 8 | 25 | - 0.018 | 0.007 | 0.019 |
| 9 | 9 | - 0.011 | 0.015 | 0.019 |
| 10 | 22 | - 0.005 | 0.021 | 0.021 |
| 11 | 3 | + 0.015 | 0.016 | 0.022 |
| 12 | 11 | + 0.008 | 0.022 | 0.023 |
| 13 | 13 | - 0.023 | 0.013 | 0.027 |
| 14 | 12 | - 0.004 | 0.028 | 0.028 |
| 15 | 21 | - 0.010 | 0.027 | 0.029 |
| 16 | 28 | - 0.002 | 0.032 | 0.032 |
| 17 | 29 | + 0.003 | 0.032 | 0.032 |
| 18 | 19 | - 0.000 | 0.033 | 0.033 |
| 19 | 30 | - 0.037 | 0.004 | 0.037 |
| 20 | 17 | - 0.024 | 0.030 | 0.039 |
| 21 | 6 | + 0.026 | 0.036 | 0.044 |
| 22 | 14 | - 0.049 | 0.007 | 0.049 |
| 23 | 20 | - 0.009 | 0.050 | 0.051 |
| 24 | 10 | - 0.065 | 0.016 | 0.067 |
| 25 | 18 | + 0.069 | 0.011 | 0.070 |
| 26 | 16 | - 0.049 | 0.059 | 0.077 |
| 27 | 23 | + 0.074 | 0.021 | 0.077 |
| 28 | 2 | + 0.139 | 0.019 | 0.140 |
| 29 | 7 | - 0.152 | 0.022 | 0.154 |
| 30 | 1 | + 0.157 | 0.020 | 0.159 |
| NC | 27 | | | |



+/- 0,10 g / 100 g pour d et 0,03 g / 100 g pour Sd

+/- 0,10 g / 100 g for d and 0,03 g / 100 g for Sd

Nb – poradové číslo

N° – číslo laboratória

Sd – smerodajná odchýlka

(prípustná hodnota od meranej hodnoty mlieka)

Tableau III : Moyennes des doubles en g / 100 g
Means of the duplicates in g / 100 g

| N° | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | 11 | 12 | 13 |
|-----------|--------------|--------------|--------------|--------------|--------------|--------------|--------------|--------------|--------------|--------------|--------------|--------------|--------------|
| 22 | 5.040 | 5.020 | 4.980 | 5.440 | 5.905 | 4.950 | 4.910 | 4.910 | 4.905 | 4.970 | 5.070 | 5.080 | 4.980 |
| M | 5.082 | 5.036 | 4.992 | 5.432 | 5.882 | 4.942 | 4.892 | 4.920 | 4.930 | 5.003 | 5.082 | 5.063 | 4.971 |
| REF. | 5.082 | 5.036 | 4.992 | 5.432 | 5.882 | 4.942 | 4.892 | 4.920 | 4.930 | 5.003 | 5.082 | 5.063 | 4.971 |
| E.T. | 0.060 | 0.058 | 0.046 | 0.031 | 0.037 | 0.059 | 0.060 | 0.057 | 0.060 | 0.059 | 0.057 | 0.061 | 0.060 |

M = moyennes par niveau

REF. = valeur de référence


E.T. = écarts types par niveau

*: valeur éliminée sur test de Grubbs à 5 %

stípec 1 až 13 – číslo vzorky

REF. – hodnota francúzskej vzorky

E.T. – odchýlka od štandardu

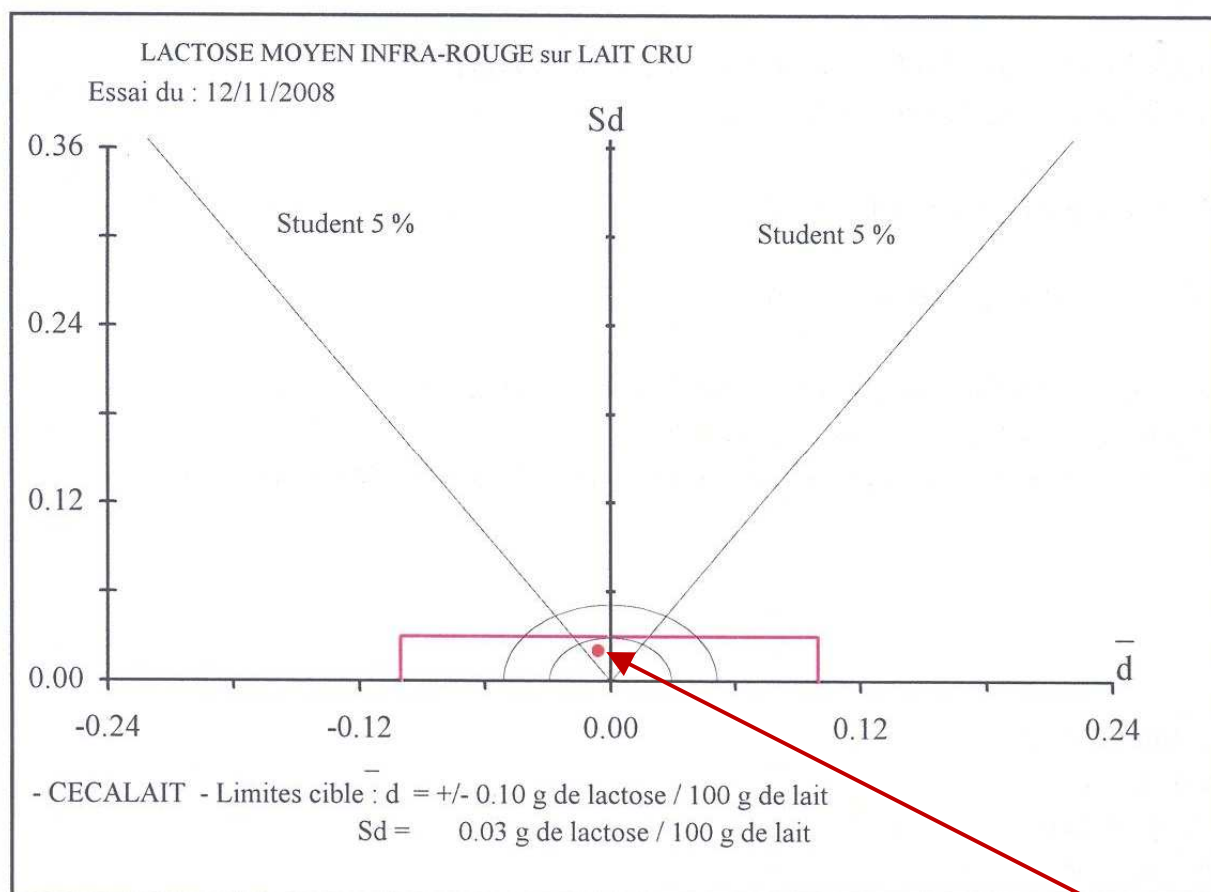

CLRM

Pozn. Vo farebnom obdĺžniku mali byť namerané hodnoty